

---

---

**Plastics — Determination of thermal  
conductivity and thermal diffusivity —**

**Part 4:  
Laser flash method**

*Plastiques — Détermination de la conductivité thermique et de la  
diffusivité thermique —*

*Partie 4: Méthode flash laser*





**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2017, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Ch. de Blandonnet 8 • CP 401  
CH-1214 Vernier, Geneva, Switzerland  
Tel. +41 22 749 01 11  
Fax +41 22 749 09 47  
copyright@iso.org  
www.iso.org

# Contents

	Page
<b>Foreword</b> .....	<b>iv</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Principle</b> .....	<b>2</b>
<b>5 Apparatus</b> .....	<b>2</b>
<b>6 Test specimen</b> .....	<b>5</b>
6.1 Shape and dimension of the specimen.....	5
6.2 Preparation and conditioning of test specimen.....	5
6.3 Coating the specimen.....	5
<b>7 Calibration and verification</b> .....	<b>6</b>
7.1 Calibration of apparatus.....	6
7.2 Verification of apparatus.....	6
<b>8 Procedure</b> .....	<b>6</b>
<b>9 Data analysis</b> .....	<b>8</b>
<b>10 Uncertainty</b> .....	<b>9</b>
<b>11 Test report</b> .....	<b>9</b>
<b>Annex A (informative) Correction for finite pulse duration</b> .....	<b>11</b>
<b>Annex B (informative) Alternative methods of calculating thermal diffusivity</b> .....	<b>12</b>
<b>Annex C (normative) Samples and test specimen preparation for injection mouldable thermoplastics and thermosets</b> .....	<b>13</b>
<b>Bibliography</b> .....	<b>17</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical-chemical properties*.

This second edition cancels and replaces the first edition (ISO 22007-4:2008), [Annex C](#) of which has been technically revised.

A list of all parts in the ISO 22007 series can be found on the ISO website.

# Plastics — Determination of thermal conductivity and thermal diffusivity —

## Part 4: Laser flash method

### 1 Scope

This document specifies a method for the determination of the thermal diffusivity of a thin solid disc of plastics in the thickness direction by the laser flash method. This method is based upon the measurement of the temperature rise at the rear face of the thin-disc specimen produced by a short energy pulse on the front face.

The method can be used for homogeneous solid plastics as well as composites having an isotropic or orthotropic structure. In general, it covers materials having a thermal diffusivity,  $\alpha$ , in the range  $1 \times 10^{-7} \text{ m}^2\cdot\text{s}^{-1} < \alpha < 1 \times 10^{-4} \text{ m}^2\cdot\text{s}^{-1}$ . Measurements can be carried out in gaseous and vacuum environments over a temperature range from  $-100 \text{ }^\circ\text{C}$  to  $+400 \text{ }^\circ\text{C}$ .

NOTE For inhomogeneous specimens, the measured values can be specimen thickness dependent.

### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO/IEC Guide 98-3, *Uncertainty of measurement — Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*

ISO 291, *Plastics — Standard atmospheres for conditioning and testing*

ISO 527-1, *Plastics — Determination of tensile properties — Part 1: General principles*

ISO 2818, *Plastics — Preparation of test specimens by machining*

ISO 22007-1, *Plastics — Determination of thermal conductivity and thermal diffusivity — Part 1: General principles*

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 22007-1 apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

— IEC Electropedia: available at <http://www.electropedia.org/>

— ISO Online browsing platform: available at <http://www.iso.org/obp>

#### 3.1 pulse width

$t_p$

duration for which the laser pulse intensity is larger than half of its maximum value

Note 1 to entry: It is expressed in seconds (s).

**3.2**  
**time origin**

$t_0$   
start of the laser pulse

Note 1 to entry: It is expressed in seconds (s).

**3.3**  
**maximum temperature rise**

$\Delta T_{\max}$   
difference between the maximum temperature reached by the rear face of the specimen after the laser pulse has passed and its steady temperature before the pulse

Note 1 to entry: It is expressed in kelvins (K).

**3.4**  
**half-rise time**

$t_{1/2}$   
time from the time origin until the rear-face temperature increases by one-half of  $\Delta T_{\max}$

Note 1 to entry: It is expressed in seconds (s).

**3.5**  
**thermogram**  
temperature versus time curve for the rear face of the specimen

**3.6**  
**thickness**  
 $d$   
dimension of the test specimen in the direction of heat transfer measurement

Note 1 to entry: It is expressed in metres (m).

## 4 Principle

One side of a flat-sheet test specimen is subjected to an energy pulse which has a very short duration compared with the half-rise time (see [6.1](#)) and a uniform spatial energy distribution. The transient temperature rise on the opposite face (rear face) is recorded as a function of time (see [Figure 1](#)). The thermal diffusivity is obtained by comparing the experimental thermogram with a theoretical model (see [Clause 9](#) and [Annex B](#)).

## 5 Apparatus

### 5.1 General

The apparatus shall be designed to obtain the thermal diffusivity as described in [Clause 4](#) and shall consist of the following main components as shown in [Figure 2](#). These are the furnace or climatic chamber with a specimen holder and temperature measurement device (e.g. thermocouple), the flash source (e.g. laser), the pulse detector, the transient detector (IR detector) and the control, data acquisition and analysis unit.

### 5.2 Furnace or climatic chamber

The furnace or climatic chamber shall meet the following requirements.

- a) The temperature range shall be appropriate to the range of materials to be studied. Depending on the range of temperature, the specimen is maintained at a constant temperature by a cryostat or by a furnace.


- b) It shall be capable of maintaining the test temperature constant to within  $\pm 0,5$  K or less for at least 30 min.
- c) The temperature measurement device shall be capable of measuring the furnace or climatic chamber temperature with a resolution of  $\pm 0,1$  K and an accuracy of  $\pm 0,5$  K or better.
- d) The furnace or climatic chamber shall be fitted with two windows, one transparent to the pulse radiation and the other transparent to the working wavelength range of the IR detector.
- e) If required, the test environment shall be vacuum or inert-gas atmosphere to avoid oxidative degradation during heating and testing of the specimen. For cryoscopic measurements, care shall be taken to avoid water condensation on the windows.

NOTE Measurement under vacuum will eliminate convection effects.

The specimen holder shall be designed to minimize thermal contact with the specimen and to suppress stray light transmitted from the laser beam to the IR detector.

The test temperature shall be measured using a calibrated temperature measurement device that is preferably in contact with the specimen or the specimen holder but at least within 1 mm of the specimen holder.


The temperature measurement device shall be designed so as not to significantly disturb the temperature field generated in the specimen by the laser pulse.

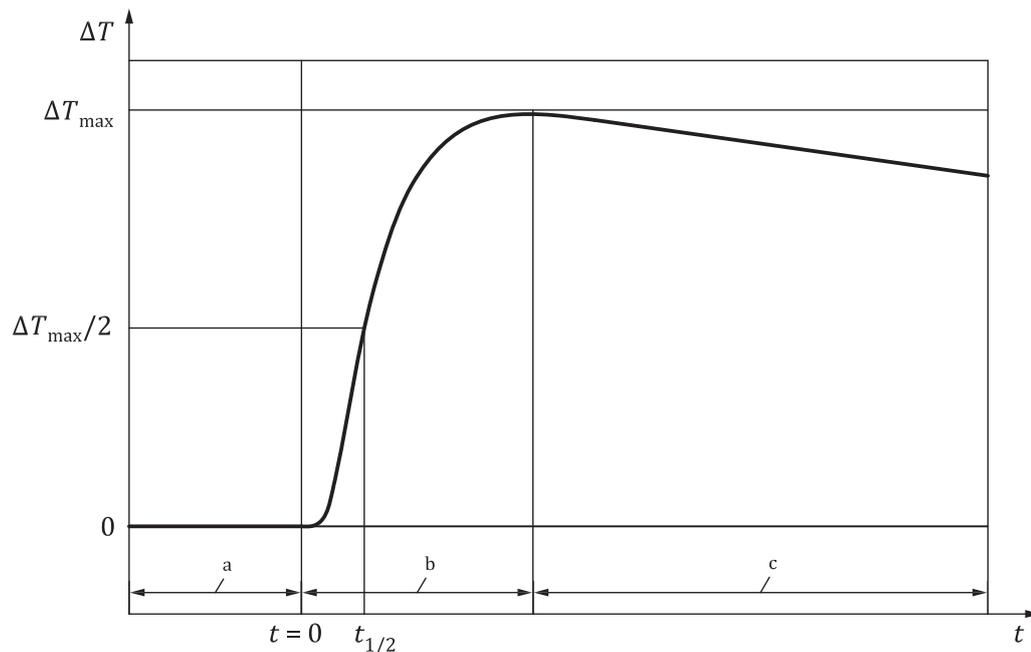

#### Key

- $t$  time
- $\Delta T$  temperature rise
- a Baseline.
- b Transient-rise period.
- c Cooling period.

**Figure 1 — Example of thermogram**

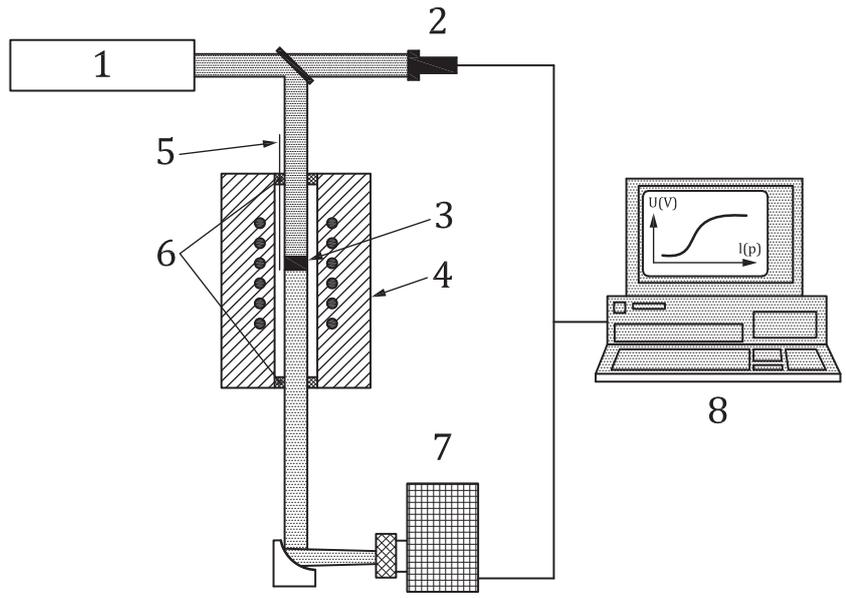

- Key**
- 1 flash source
  - 2 pulse detector
  - 3 specimen
  - 4 furnace or climatic chamber
  - 5 temperature measurement device
  - 6 windows
  - 7 transient detector
  - 8 control, acquisition and analysis unit

**Figure 2 — Schematic diagram of laser flash set-up for measuring thermal diffusivity**

**5.3 Flash source**

The energy level of the flash source shall produce a temperature rise not exceeding 3 K at the rear face of the specimen.

The spatial energy distribution of the pulse heating shall be as uniform as possible over the front face of the specimen.

The pulse duration shall be shorter than 1 ms.

The heat pulse source may be a laser (preferably) or a flash tube.

A photodiode can be used to determine the duration and form of the pulse and the time origin.

**5.4 Transient detectors**

The transient temperature rise at the rear face of the specimen shall be measured with an IR detector. The transient detector shall be able to detect a variation of 5 mK in the specimen rear face temperature. Its response shall be linear with temperature over a temperature range of at least 3 K.

The frequency response of the detector and its associated electronics (amplifiers, analogue/digital converters, etc.) shall be faster than 10 kHz. If electronic filters are used, they shall meet the requirements

defined above and shall not decrease the accuracy of temperature measurement, otherwise they could distort the shape of the temperature-time curve.

NOTE The choice of IR detector depends also on the temperature range. For the range  $-100\text{ °C}$  to  $+400\text{ °C}$ , photovoltaic or photoconductor detectors can be used.

The temperature of the rear face, or a quantity directly proportional to it (e.g. voltage), shall be measured and recorded continuously over the duration of the test. The data acquisition system, which may be analogue or digital, shall be able to sample more than 1 000 data points on the thermogram with a sampling frequency higher than  $100/t_{1/2}$ . The accuracy of the time base shall be better than  $\pm 1 \times 10^{-5}$  s.

### 5.5 Thickness measurement device

The specimen thickness shall be measured with an accuracy of  $\pm 5\text{ }\mu\text{m}$  by a calibrated thickness measurement device having a resolution of  $\pm 1\text{ }\mu\text{m}$ . For soft materials, a micrometer with reproducibly low compression is required.

## 6 Test specimen

### 6.1 Shape and dimension of the specimen

The specimen shall be a thin disc. The specimen diameter is usually from 5 mm to 20 mm. The specimen thickness shall be chosen according to the pulse width and the thermal diffusivity of the material. It shall be selected such that the pulse width is less than 0,01 of the half-rise time. Typically, the thickness will be between 0,5 mm and 3 mm. The aspect ratio of the specimen shall be chosen such that 2D effects are negligible during the test. The ratio of the diameter to the thickness shall be larger than 3:1.

The faces shall be flat and parallel. Any variation in the thickness of the specimen should preferably be less than 1 % of the mean thickness. The effect of greater non-uniformity can be estimated in the measurement uncertainty.

### 6.2 Preparation and conditioning of test specimen

The test specimen shall be representative of the material being examined and shall be prepared and handled with care. If the specimen is taken from sample pieces by cutting, care shall be taken to prevent heating, changes in molecular orientation or any other effect that may alter the sample properties.

A method for sample preparation of oriented, anisotropic specimens is specified in [Annex C](#).

The test specimen shall be conditioned prior to the measurement as specified in the relevant material standard or by a method agreed between the parties involved. Unless other conditions are specified, it is recommended that the specimen be conditioned in accordance with ISO 291.

NOTE Depending on the material and its thermal history, the method of test specimen preparation may be crucial to the consistency of the results and their significance.

### 6.3 Coating the specimen

Specimens which are not opaque to the laser radiation at the wavelength used shall be coated with an appropriate coating (a metal coating, for example) to prevent penetration of the laser beam into the specimen. The influence of the coating on the heat transfer shall be negligible (i.e. it shall have a high diffusivity and low thickness in comparison with the specimen). The total thickness of the coating shall be chosen such that the half-rise time for the coating alone is less than 2 % of the total half-rise time for the specimen.

NOTE 1 The half-rise time,  $t_{1/2}$ , for the coating can be simply calculated from its thickness,  $d$ , and thermal diffusivity,  $\alpha$ , using [Formula \(1\)](#), a rearranged form of [Formula \(B.1\)](#):

$$t_{1/2} = 0,13879 \frac{d^2}{\alpha} \quad (1)$$

NOTE 2 Both sides of the specimen can be coated with a thin opaque black layer (i.e. a layer of graphite) to optimize the absorption of the energy pulse and the emission of thermal radiation.

## 7 Calibration and verification

### 7.1 Calibration of apparatus

The laser flash technique is an absolute method which allows the user to perform measurements that are directly traceable to primary SI units (such as temperature, time, length and voltage) without calibration using reference materials. All elements of the laser flash apparatus shall be calibrated separately, as follows.

- Calibrate the micrometer used to measure the specimen thickness.
- Calibrate the temperature measurement device used to measure the steady-state temperature of the specimen.
- Calibrate the time base and the voltage of the data acquisition system used to measure the signal coming from the IR detector.
- Calibrate the IR detector in order to be able to observe the transient temperature change at the rear face of the specimen rather than the transient spectral irradiance. Perform this calibration mainly for temperatures lower than 200 °C where nonlinear behaviour of the output temperature cannot be neglected (see ISO 18755[1]). If this calibration is not possible (e.g. because the IR detector is inaccessible or due to differences between the optical paths of the IR detector calibration configuration and the thermal-diffusivity measurement configuration), the effects of nonlinearity have to be taken into account in the uncertainty of measurement.

### 7.2 Verification of apparatus

The apparatus should preferably be verified periodically by measuring the thermal diffusivity of one or more reference materials covering the range of thermal diffusivities of the materials to be tested. If the measured values differ by more than 5 % from the reference values, recalibrate the various items of apparatus in accordance with 7.1.

Verification can be carried out by measurements on materials which have well-defined and reproducible thermal properties such as Armco<sup>1)</sup> iron, Poco<sup>1)</sup> graphite, Pyroceram 9606<sup>1)</sup> or poly(methylmethacrylate) (PMMA). Pyroceram 9606 (a ceramic material) has been certified for thermal-diffusivity measurements as part of an international programme involving national metrology institutes[2]. This certified reference material is available from IRMM (Institute for Reference Materials and Measurements)[3].

It is recommended that the reference materials be chosen so that their properties (half-rise time and thermal diffusivity) are close to those of the materials to be tested.

## 8 Procedure

**8.1** Switch on the equipment at least 1 h prior to any testing to allow it to reach equilibrium.

---

1) Armco, Poco and Pyroceram 9606 are examples of products available commercially. This information is given for the convenience of users of this document, and does not constitute an endorsement by ISO of the products named.

**8.2** Measure the thickness of the specimen at ambient temperature, using a calibrated thickness measurement device. If a specimen coating is used, the specimen-thickness measurement shall be made before coating.

**8.3** Mount the specimen in its holder and put this assembly in the furnace or climatic chamber.

**8.4** If required, establish a vacuum or an inert-gas environment in the furnace or climatic chamber.

**8.5** Set the furnace or climatic chamber to the desired temperature and wait until the stability of the specimen temperature is better than 0,05 K/s.

**8.6** Measure the steady-state temperature of the specimen.

**8.7** Calculate the specimen thickness at the test temperature, taking into account the change in thickness due to thermal expansion.

**8.8** Irradiate the specimen with the laser pulse, taking adequate safety precautions. Care shall be taken to ensure that the laser beam does not cause any local degradation of the specimen. The specimen shall be inspected after removal from the instrument to check for any signs of degradation.

**8.9** Measure and record continuously the temperature of the rear face of the specimen or a quantity directly proportional to it before, during and after the laser pulse. The thermogram obtained shall include the baseline, the transient-rise period and the cooling period (see [Figure 1](#)).

**8.10** If necessary, measure the time form of the laser pulse applied in [8.8](#) in order to correct for the effect of the finite duration of the pulse (for guidance see [Annex A](#)).

**8.11** From the thermogram obtained, calculate the thermal diffusivity in accordance with [Clause 9](#).

**8.12** Repeat at least three times the procedures described from [8.8](#) to [8.11](#) at the same temperature and calculate the average value of the thermal diffusivity and the repeatability of the measurements.

The analysis assumes that the specimen is homogeneous. If there are any doubts about the homogeneity, it is recommended that measurements be performed on two specimens with a thickness ratio of about 1:2. If the same diffusivity values are obtained, the effect of inhomogeneity can be assumed to be negligible.

**8.13** Change the test temperature to the next desired temperature and repeat steps [8.5](#) to [8.12](#).

If testing is being carried out at several temperatures, it is recommended that an increasing rather than decreasing temperature profile be used as this will minimize or avoid the effect of distortion of the specimen on the results, as distortion is more likely to occur at higher temperatures.

If testing at elevated temperatures, it is recommended that the effect of possible changes in the specimen at such temperatures be investigated. This can be done by carrying out a test at ambient temperature both before and after the required series of tests. If there is a difference in the results obtained, consideration shall be given to reducing the time at elevated temperature for each specimen.

Care shall be taken to avoid testing at temperatures at which the specimen may undergo a transformation (e.g. first- or second-order transformation, crystal transformation or glass transition) during the test.

**NOTE** The test temperature is a nominal temperature that can be associated with the measured thermal-diffusivity value as this value is determined under higher transient temperatures due to the heating effect of the laser pulse. An extrapolation procedure<sup>[4]</sup> can be used to calculate the “intrinsic thermal diffusivity” at the test temperature corresponding to the thermal diffusivity that would be measured for a laser pulse of zero energy.

## 9 Data analysis

The analysis of the rear-face temperature curve and the calculation of the thermal diffusivity shall be carried out as follows.

- a) If the half-rise time,  $t_{1/2}$ , is shorter than 100 times the pulse width, correct the time scale for the finite pulse time effect (for guidance, see [Annex A](#)).
- b) Determine the baseline and the maximum of the curve to calculate the maximum temperature rise,  $\Delta T_{\max}$ . If the baseline shows a drift, correct the thermogram by subtracting the extrapolated baseline.
- c) Normalize the rear-face temperature rise curve by dividing all temperature rise values by  $\Delta T_{\max}$ .
- d) Calculate the thermal diffusivity from the normalized thermogram, using the partial time moments method[5] described below, or any other suitable method, as well as the thickness,  $d$ , corrected for thermal expansion.

The “partial time moments” method recommended in this document has a low sensitivity to measurement noise. It uses only the rising part of the thermogram, which is highly sensitive to thermal diffusivity. Other methods may be used as long as their uncertainties are calculated. [Annex B](#) gives examples of such methods of calculation.

NOTE 1 Additional information on calculation methods, data analysis and sources of error can be found in ISO 18755[1]. Since ISO 18755 refers to ceramics, not all the details presented therein are necessarily relevant to the testing of plastics.

In the partial time moments method, the thermal diffusivity is given by [Formula \(2\)](#):

$$\alpha = \frac{d^2 F(m_{-1})}{m_0} \quad (2)$$

The two partial time moments,  $m_0$  and  $m_{-1}$ , are defined by [Formulae \(3\)](#) and [\(4\)](#):

$$m_0 = \int_{t_{0,1}}^{t_{0,8}} \frac{\Delta T(t)}{\Delta T_{\max}} dt \quad (3)$$

and

$$m_{-1} = \int_{t_{0,1}}^{t_{0,8}} \frac{1}{t} \times \frac{\Delta T(t)}{\Delta T_{\max}} dt \quad (4)$$

where

$\Delta T(t)$  is obtained from the experimental thermogram;

$t_{0,1}$  and  $t_{0,8}$  are the times required from the initiation of the pulse for the rear face of the specimen to reach 10 % and 80 % of  $\Delta T_{\max}$ .

The function  $F(m_{-1})$  is defined by [Formulae \(5\)](#) and [\(6\)](#):

$$\text{For } 0,44 > m_{-1} > 0,27: F(m_{-1}) = 0,085\ 48 - 0,314 (0,548\ 6 - m_{-1}) + 0,500 (0,548\ 6 - m_{-1})^{2,63} \quad (5)$$

$$\text{For } m_{-1} > 0,44: F(m_{-1}) = -0,081\ 9 + 0,305 m_{-1} \quad (6)$$

NOTE 2 Values of  $m_{-1}$  less than 0,27 do not have any physical significance.

This calculation method can be used if the following conditions are satisfied:

- the duration of the laser pulse is short compared with the time characteristic for thermal diffusion (i.e. pulse width  $<1\%$  of  $t_{1/2}$ ) or, if not, a correction is applied to the time scale in accordance with [Annex A](#);
- the front face of the specimen is uniformly heated by the laser pulse;
- the specimen is homogeneous;
- the specimen is opaque to the laser radiation at the wavelength used.

NOTE 3 The potential effect of non-uniformity of the pulse on the calculated thermal diffusivity can usually be assumed to be negligible due to the use of an IR detector to detect the transient temperature rise of the specimen rear face. However, if needed, the laser beam could be made more uniform by using beam-homogenizing optics.

NOTE 4 The assumption of opacity of the specimen is implicitly satisfied by the deposit of an appropriate coating on its two faces.

## 10 Uncertainty

The relative expanded uncertainty (confidence level of 95 %) of the thermal-diffusivity determination by the laser flash method with the partial time moments method is estimated to be from  $\pm 3\%$  to  $\pm 5\%$ <sup>[6]</sup> between ambient temperature and 400 °C (depending on the material and the temperature). It has been calculated in accordance with the ISO/IEC Guide 98-3. On the basis of the results of five successive measurements performed under the same conditions, the repeatability of the method is better than 1 %.

## 11 Test report

The test report shall include the following information:

- a) a reference to this document, i.e. ISO 22007-4;
- b) the date of the test;
- c) all details necessary for complete identification of the sample tested (type, batch number, etc.), including its thermal history;
- d) the shape and dimensions (diameter and thicknesses at room temperature and at each test temperature, giving the method of calculation of the thicknesses at the test temperatures) of the specimens and the number of specimens tested;
- e) details of sample and specimen preparation;
- f) whether a coating was used and, if so, the coating material and coating procedure and the thickness of the coating);
- g) the wavelength and duration of the laser pulse;
- h) the type of detector used for measuring the transient temperature rise of the specimen rear face;
- i) the type of furnace used and its temperature range (or a statement to the effect that a climatic chamber was used);
- j) the measurement conditions, such as the test temperature(s), in degrees Celsius, and the furnace or climatic chamber atmosphere;
- k) the method(s) used to calculate the thermal diffusivity and estimate corrections (e.g. due to heat losses and the finite pulse duration);
- l) the thermal-diffusivity value(s) obtained, in square metres per second;

- m) any additional information or details of operations not specified in this document, which may be important for assessment of the results.

## Annex A (informative)

### Correction for finite pulse duration

All the methods used to calculate thermal diffusivity assume that the laser pulse is similar to a Dirac function. However, if the duration of the pulse cannot be neglected (see [Clause 9](#)), the effect of the finite pulse time should be corrected for.

For the methods of calculation based on the use of the half-rise time,  $t_{1/2}$ , a first approach consists in calculating the thermal diffusivity, assuming a Dirac function pulse, and applying a correction to the value obtained. By specifying the shapes of pulses, several authors[7],[8],[9] have proposed analytical relationships to estimate this correction.

A more general method consists in shifting the time origin to the centroid,  $t_g$ , of the laser pulse and calculating the thermal diffusivity considering the pulse as a Dirac function. In this case, the waveform of the laser pulse is measured by a detector having a response faster than 10  $\mu\text{s}$  and the position of the centroid is calculated directly from the observed waveform. This method, proposed initially by Azumi and Takahashi[10] for adiabatic experiments, has been extended to non-adiabatic ones by Degiovanni[11].

## Annex B (informative)

### Alternative methods of calculating thermal diffusivity

All methods of calculating thermal diffusivity are based on the mathematical solution of the heat conduction equation with appropriate initial and boundary conditions. The original method proposed by Parker et al.<sup>[12]</sup> is based on an analytical model corresponding to an adiabatic experiment, on the basis of which the thermal diffusivity is calculated from the half-rise time,  $t_{1/2}$ .

In the case of an adiabatic experiment, the thermal diffusivity is calculated simply from the thickness,  $d$ , and the half-rise time,  $t_{1/2}$ , as follows:

$$\alpha = 0,13879 \frac{d^2}{t_{1/2}} \quad (\text{B.1})$$

The use of this method, which neglects heat losses, can generate significant systematic errors in thermal diffusivity determinations. It is not a suitable method for polymers because of their low thermal diffusivity and the test cannot really be considered adiabatic.

Some methods are based on an improvement of Parker's method, introducing correction factors in the calculation of the thermal diffusivity to take into account the unavoidable heat losses. They use one or several characteristic points on the experimental curve. Among them, Cape and Lehman's method<sup>[13]</sup>, Cowan's method<sup>[14]</sup> and Clark and Taylor's method<sup>[15]</sup> are the most commonly used.

With the advances in modern data acquisition, methods based on the analysis of a part (i.e. the partial time moments method of Degiovanni and Laurent<sup>[5]</sup>) or the whole of the temperature response (i.e. the technique proposed by Gembarovic et al.<sup>[16]</sup> using a least-squares method) are increasingly utilized. These calculation methods are generally based on minimizing the difference between the measured values and the theoretical values obtained from a mathematical model. They differ either by the analytical model used or by the way in which they compare the measured temperature rise versus time recordings with the analytical curve.

## Annex C (normative)


### Samples and test specimen preparation for injection mouldable thermoplastics and thermosets

#### C.1 General

The purpose of this annex is to provide a comparable sample preparation for the measurement of the directional thermal conductivity of injection mouldable thermoplastics and thermoset. This is necessary, because the thermal conductivity and thermal diffusivity values are influenced by the orientation of the filler particles, the sample shape, dimension and preparation. The preparation of the test specimen out of these samples (plates) also has an influence on the above values.

#### C.2 Sample shape and dimension

[Figure C.1](#) shows an example of a plate.

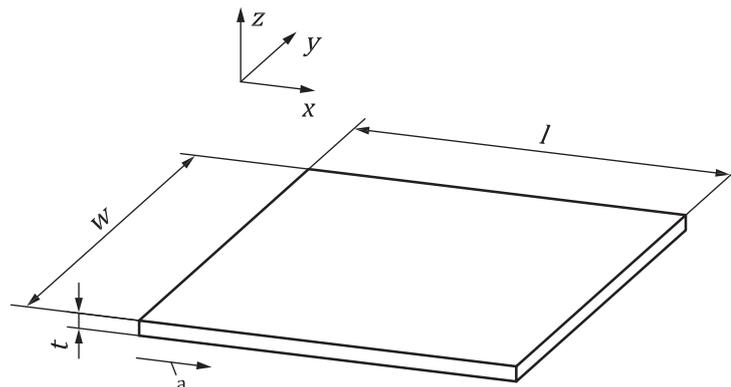

#### Key

$w$	width	$z$	measuring direction: through-plane
$l$	length	$y$	measuring direction: in-plane — perpendicular
$t$	thickness	$x$	measuring direction: in plane — parallel
$a$	Flow direction (injection direction).		

**Figure C.1 — Example of sample**

Minimum dimensions of the plates:

- width  $w$ : 40 mm
- length  $l$ : 50 mm
- thickness  $t$ : 2 mm

The film-gate shall be over the whole width  $w$  of the sample (plate).

### C.3 Sample manufacturing

Plates shall preferably be injection-moulded from granulate. The injection moulding conditions shall be in accordance with the relevant International Standard for the material or, if none exists, agreed between the interested parties.

Strict control of all conditions of the samples (plates) preparation is essential to ensure that all test specimens in a set are actually in the same state.

Plates shall be coplanar and of uniform thickness. All surfaces shall be free from visible flaws, scratches or other imperfections.

Test specimens from finished goods shall be taken from flat areas or zones having minimum curvature.

Plates should not be machined to reduce their thickness. Test specimens with machined surfaces will not give results comparable to specimens having non-machined surfaces.

If samples (plates) have to be compression-moulded, extruded or machined in accordance with ISO 2818 it shall be noted in the test report. In general injection moulded samples are preferred.

### C.4 Sample inspection

The sample inspection shall be done in accordance with ISO 527-1.

### C.5 Sample anisotropy

Injection moulded samples (plates), as well as finished component parts, exhibit some degree of anisotropy as a result of flow-induced orientation.


The direction dependence of the thermal properties can be assessed by cutting specimens parallel and normal to the flow direction characterizing the moulding process. In the absence of information on such directions, specimens shall be machined in directions as agreed between the interested parties.

- in flow-direction, in-plane: x-direction (see [Figure C.1](#));
- perpendicular to flow-direction, in-plane: y-direction (see [Figure C.1](#));
- perpendicular to flow-direction, through-plane: z-direction (see [Figure C.1](#)).


### C.6 Location and preparation of the test specimen

#### C.6.1 General

All test specimens shall be prepared from the middle of the sample with regard to the direction of flow (see [Figure C.2](#) and [Figure C.3](#)).

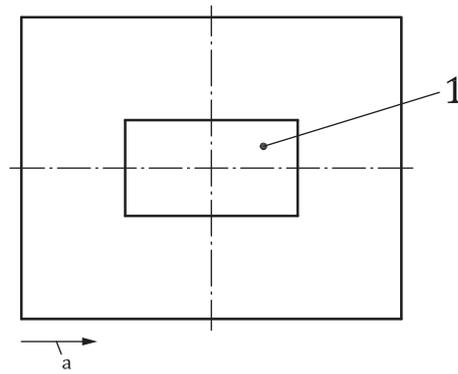**Key**

- 1 specimen location  
a Injection direction.

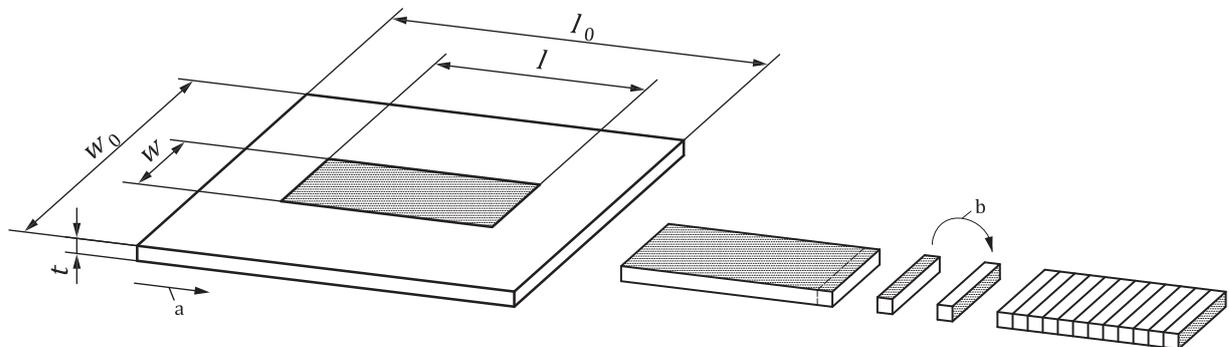**Figure C.2 — Placement of test specimen****Key**

- $w_0$  width of plate  
 $l_0$  length of plate  
 $t$  thickness of plate  
a Flow direction (injection direction).  
b Rotation of stripes by 90°.
- $w$  width of test specimen  
 $l$  length of test specimen including cutting scrap

**Figure C.3 — Preparation procedure of test specimen**

Depending on the measuring equipment, the dimensions of the sample specimen can vary. The following is one option for a special sample geometry.

To measure in in-plane direction, a platelet of 28 mm × 12,7 mm × 2 mm shall be cut or punched from the middle of the sample either parallel (x-direction) or perpendicular (y-direction) to the flow direction. Stripes of 12,7 mm × 2 mm × 2 mm of this platelet are obtained by sawing. These stripes shall be turned by 90° and clamped as a laminate into a specimen fixture. The resulting laminated test specimen shows a minimum size in accordance with this document. The stripes shall not be deformed during clamping. After clamping, the surface of the laminate shall be grinded to obtain a uniform thickness. Excessive heat input shall be avoided.

**C.6.2 Measuring direction in through-plane direction (z-direction)**

The test specimen in accordance with this document shall be prepared directly from the plate by cutting or punching. The upper and lower surface of the test specimen shall not be changed. Excessive heat input shall be avoided.

### **C.6.3 Measuring direction in in-plane direction (x-, y-direction):**

The anisotropy of the thermal conductivity in in-plane directions can be determined by preparing specimens either parallel (for example as shown in [Figure C.3](#)) or perpendicular to the flow direction.

## **C.7 Test report**

The test report shall include the following information in addition to the test report specified in [Clause 11](#):

- details of sample manufacturing and test specimen preparation including information on measuring direction in regard to the flow-direction;
- the method and corresponding standard used to obtain the specific heat of the test specimen;
- all deviations from this annex.

## Bibliography

- [1] ISO 18755, *Fine ceramics (advanced ceramics, advanced technical ceramics) — Determination of thermal diffusivity of monolithic ceramics by laser flash method*
- [2] SALMON D., BAXENDALE S., GROBOTH G., HAY B., HAMMERSCHMIDT U., BRANDT R., SINNEMA S., BAILLIS D. *The certification of thermal conductivity and diffusivity properties of Pyroceram 9606 as a reference material up to 1 000 °C, HTCRM, Certification Report (2003)*
- [3] <http://www.irmm.jrc.be>
- [4] AKOSHIMA M., & BABA T. Thermal Diffusivity Measurements of Candidate Reference Materials by the Laser Flash Method. *Int. J. Thermophys.* 2005, **26** (1) pp. 151–163
- [5] DEGIOVANNI A., & LAURENT M. Une nouvelle technique d'identification de la diffusivité thermique par méthode flash. *Rev. Phys. Appl. (Paris)*. 1986, **21** pp. 229–237
- [6] HAY B., FILTZ J.-R., HAMEURY J., RONGIONE L. Uncertainty of Thermal Diffusivity Measurements by Laser Flash Method. *Int. J. Thermophys.* 2005, **26** (6) pp. 1883–1898
- [7] HECKMAN R.C. Finite pulse-time and heat-loss effects in pulse thermal diffusivity measurements. *J. Appl. Phys.* 1973, **44** (4) pp. 1455–1460
- [8] LARSON K.B., & KOYAMA K. Correction for finite-pulse-time effects in very thin samples using the flash method of measuring thermal diffusivity. *J. Appl. Phys.* 1967, **38** (2) pp. 465–474
- [9] TAYLOR R.E., & CLARK L.M. Finite pulse time effects in flash diffusivity method. *High Temp. High Press.* 1974, **6** pp. 65–72
- [10] AZUMI T., & TAKAHASHI Y. Novel finite pulse-width correction in flash thermal diffusivity measurement. *Rev. Sci. Instrum.* 1981, **52** (9) pp. 1411–1413
- [11] DEGIOVANNI A. Correction de longueur d'impulsion pour la mesure de la diffusivité thermique par la méthode flash. *Int. J. Heat Mass Transfer.* 1987, **30** (10) pp. 2199–2200
- [12] PARKER W.J., JENKINS R.J., BUTLER C.P., ABBOT G.L. Flash method of determining thermal diffusivity, heat capacity and thermal conductivity. *J. Appl. Phys.* 1961, **32** (9) pp. 1679–1684
- [13] CAPE J.A., & LEHMAN G.W. Temperature and finite pulse-time effects in the flash method for measuring thermal diffusivity. *J. Appl. Phys.* 1963, **34** (7) pp. 1909–1913
- [14] COWAN R.D. Pulse method of measuring thermal diffusivity at high temperatures. *J. Appl. Phys.* 1963, **34** (4) pp. 926–927
- [15] CLARK L.M., & TAYLOR R.E. Radiation loss in the flash method for thermal diffusivity. *J. Appl. Phys.* 1975, **46** (2) pp. 714–719
- [16] GEMBAROVIC J., VOZAR L., MAJERNIK V. Using the least square method for data reduction in the flash method. *Int. J. Heat Mass Transfer.* 1990, **33** (7) pp. 1563–1565



This page has been left intentionally blank.